


















**BIO COMPOSANTS
MÉDICAUX**

biolight PLUS

TUTORIAL MULTI-POSTS BIOLIGHT PLUS

- 1  Isolate the preparation using rubber dam
- 2  Remove gutta percha to a depth of at least 1.5 times the coronal height, using ultrasonics with a diamond coated tip
- 3  Leave a 5 mm minimum apical stop
- 4  Rinse and air dry
- 5  Eliminate any humidity with paper points
- 6  Clip the template over the x-ray sensor
- 7  First measure the canal width at entry to determine the size and the apical stop
- 8  Etch all surfaces that will be bonded. Rinse and air dry
- 9  Remove any residual humidity with absorbent paper points
- 10  Apply dual-cure dentine bonding agent to the etched surfaces. Air dry and absorbent paper points
- 11  Backfill the canal beginning at the apical stop. Overfill onto the prepared coronal surfaces
- 12  Insert the sleeve into the Biolight Plus
- 13  Insert the ultra-fine tip into the sleeve
- 14  Pull the Biolight Plus multi-post to expose 2/3 of its total length
- 15  Inject the resin cement until it exudes through the sleeve exit



BIO COMPOSANTS MÉDICAUX

215, route de Bavonne - ZA le Talamud
38140 Saint-Blaise-Du-Buis
+33 (0)4 76 07 79 57


dentalbcm.com
contact@biomedicaux.com




**BIO COMPOSANTS
MÉDICAUX**

biolight PLUS


TUTORIAL MULTI-POSTS BIOLIGHT PLUS

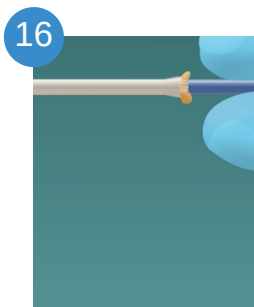


Push the Biolight Plus back into the sleeve, while maintaining pressure on the syringe

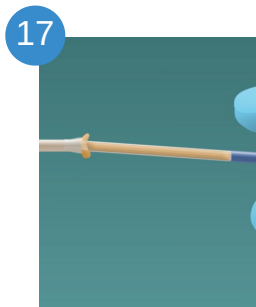


Let go of the Biolight and continue to inject: the biolight will eject from the sleeve, fully impregnated

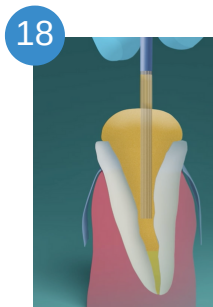


Insert the Biolight into the canal. Do not use excessive force to push towards the apical stop

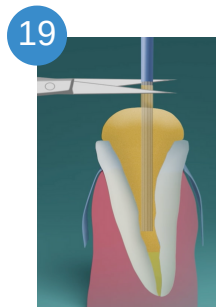


Using fine scissors, remove the sheath by cutting across the post strands

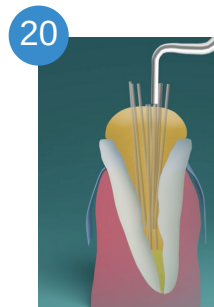


Use a condenser to vertically push down the number of strands

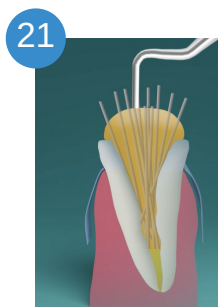


Move the remaining strands towards the periphery of the canal as much as possible

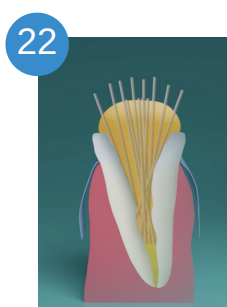

Allow for complete curing of the resin cement as per manufacturer's specifications

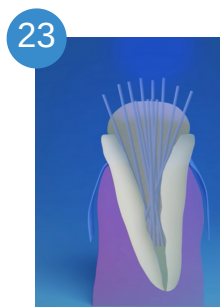

Light cure to complete the polymerization

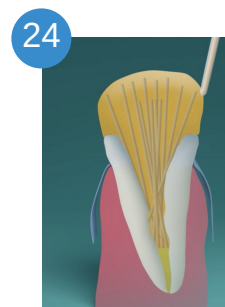

Complete the core build-up as necessary



Medical device for dental treatment, reserved for healthcare professionals.
Please read the instructions on the leaflet or on the label carefully before use.
Classe IIA (CE marking certified by SGS) CE 1639.



BIO COMPOSANTS MÉDICAUX

215, route de Bavonne - ZA le Talamud
38140 Saint-Blaise-Du-Buis
+33 (0)4 76 07 79 57

dentalbcm.com
contact@biomedicaux.com